

QUICK START GUIDE



290 Series HIPOT TESTERS

Models: 294, 295, 296, 297, 298



SAFETY CHECKLIST

- S**urvey the test station. Make sure it is safe & orderly.
- A**lways keep unqualified/unauthorized personnel away from the test area.
- F**amiliarize yourself with safety protocols in the event of a problem.
- E**xercise caution and never touch products or connections during a test.
- T**rain operators. Connect the return lead first and never touch clips directly.
- Y**ou should always know when a test is being performed.

See How Simple
Using Your Tester
Can Be

Watch the Quick
Start Video



WARNING: THIS GUIDE WAS CREATED FOR OPERATORS HAVING SOME FAMILIARITY WITH ELECTRICAL SAFETY TESTING. AN ELECTRICAL SAFETY TESTER PRODUCES VOLTAGES AND CURRENTS THAT CAN CAUSE HARMFUL OR FATAL ELECTRIC SHOCK. TO PREVENT ACCIDENTAL INJURY OR DEATH, THESE SAFETY PROCEDURES MUST BE STRICTLY OBSERVED WHEN HANDLING AND USING A TEST INSTRUMENT.

TESTER SETUP



WARNING: LOCATE A SUITABLE TESTING AREA WITH A THREE-PRONG, GROUNDED OUTLET. BE SURE THAT YOUR THREE-PRONG OUTLET HAS BEEN TESTED FOR PROPER WIRING. READ THE SAFETY CHECKLIST OF THIS GUIDE BEFORE STARTING TO TEST.



- 1 Connect the female end of the standard NEMA style line power cord into the input power receptacle on the rear panel of the tester. Plug the male end of the cord into a grounded power source.

Grounded
Power
Source




- 2 Connect the Interlock Disable Key into the Signal Input connector on the rear panel of the tester.
This is required to run a test.



- 3 Turn the POWER switch ON.


Upon start up an initial screen will appear briefly. After two seconds the Home screen will appear as shown below. Tests are performed from the Home screen.

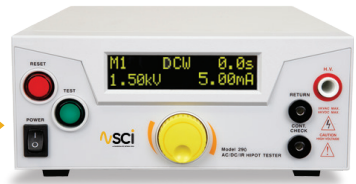


Home Screen

SETTING TEST MEMORIES

If you wish to have multiple test setups, you will need to begin by choosing a Memory Location (M1 - M5) for each test, (up to 10 optional memories).

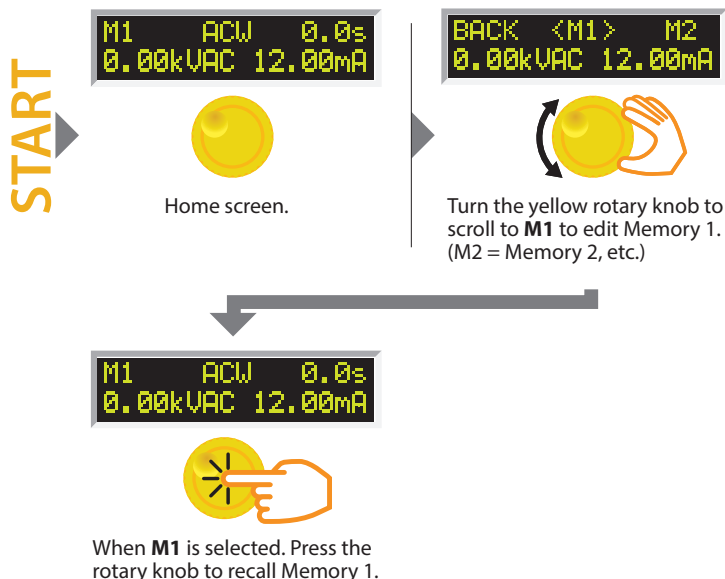

EDIT TEST PARAMETERS

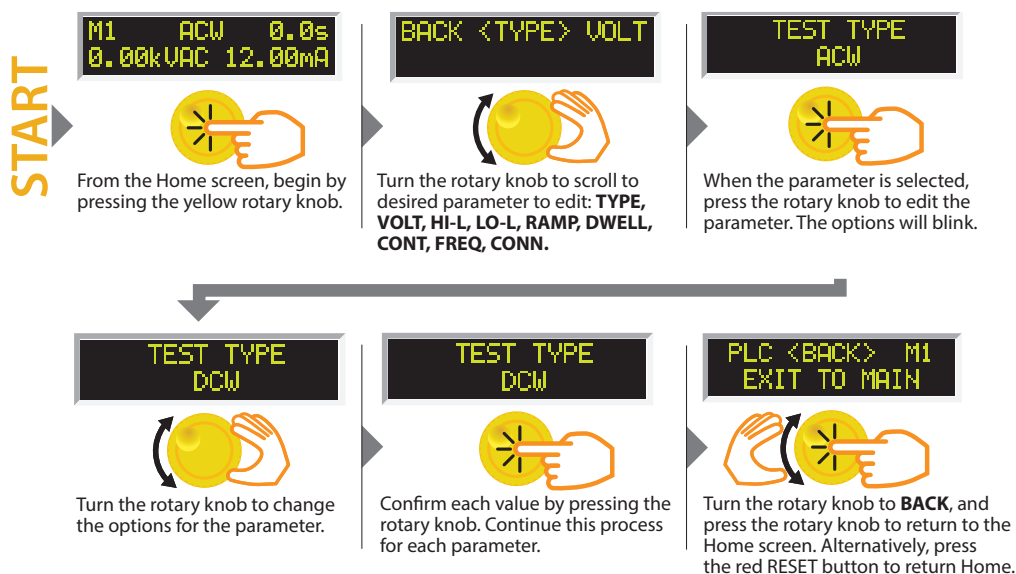

PERFORM AN ACW WITH GROUND CONTINUITY

You can easily perform an AC/DC Withstand test with a Ground Continuity check. Test Class I products through the use of the adapter box (P/N 99-10001-01) and ground return lead. To enable this function, you will need to set the tester to run either an AC or DC Hipot test.

START

M1 ACW 0.0s
0.00kVAC 12.00mA



From the home screen, begin by pressing the yellow rotary knob.

BACK <TYPE> VOLT
0.00kVAC 12.00mA



Turn the yellow rotary knob to scroll to **TYPE**.

TEST TYPE
ACW



When the parameter is selected, Press the rotary knob to edit the parameter. The options will blink.

TEST TYPE
DCW



Turn the rotary knob to change the options for the parameter, **AC or DC**.

TEST TYPE
DCW



Confirm by pressing the rotary knob.

DWLL <CONT> FREQ
OFF



Turn the rotary knob to **CONT**, and Press the knob to select.

CONTINUITY
OFF



When **CONT** is selected. Press the rotary knob to edit the Continuity setting. The options will blink.

CONTINUITY
ON



Turn the rotary knob to change the Continuity setting to **ON**. Confirm by pressing the rotary knob.

BACK <HI-L> LO-L
1.50Ω



When done, you will be prompted to enter a value for HI-Limit.

HI-L <LO-L> OFFS
0.00Ω



Then enter a value for LO-Limit.

LO-L <OFFS> BACK
0.00Ω



Then enter a value for Offset.

OFFS <BACK> HI-L
EXIT TO MAIN



When done, select **BACK** to return to the previous menu. Alternatively, press the red **RESET** button to return home.



WARNING: DO NOT TOUCH THE DEVICE UNDER TEST ONCE YOU START THE TEST.


TEST CONNECTION

Adapter Box Connections

To increase operator safety, you may elect to use an adapter box for products terminating in either a two-prong or three-prong line cord. **If using an adapter box**, follow these instructions to safely connect a DUT.

NOTE: Be sure to enable the Ground Continuity test before moving forward. See page 3.

- 1 Plug the black lead from the adapter box (P/N 99-10001-01) into the CONT. CHECK terminal located on the front panel.
- 2 Plug the white lead from the adapter box into the H. V. output terminal located on the front panel.
- 3 Plug the black ground return lead (P/N 102-069-904) to the front panel RETURN terminal. Connect the clip end of the lead to the dead metal on the chassis of the DUT. Check to ensure a solid connection is made between the DUT and the return clip.
- 4 Plug the line cord of the DUT into the adapter box receptacle.

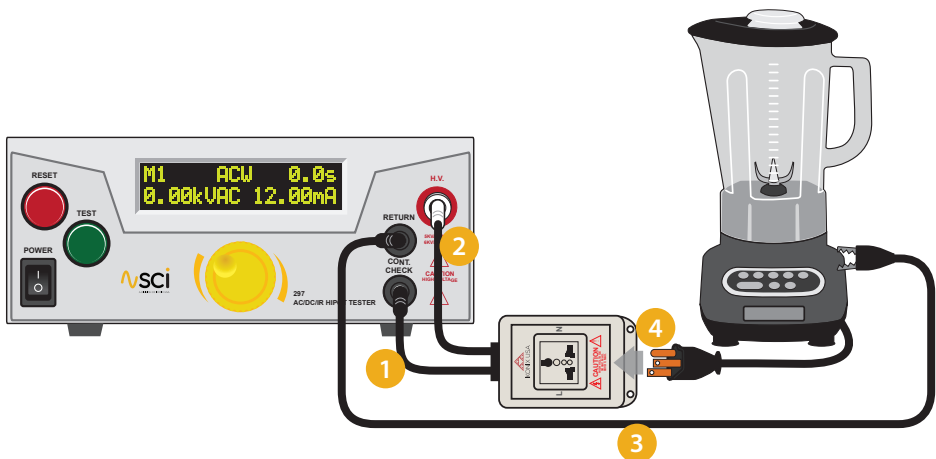

TEST CONNECTION




WARNING: DO NOT TOUCH THE DEVICE UNDER TEST ONCE YOU START THE TEST.

DUT Connections


If you elect to use test leads, follow these instructions to safely connect a DUT.

- 1 Plug the black ground return lead (P/N 102-069-904) into the RETURN terminal located on the front panel of the tester.
- 2 Plug the high voltage lead (P/N 102-055-913) into the H.V. terminal on the front panel of the tester.
- 3 Plug the continuity lead to the CONT. CHECK terminal on the front panel of the tester. (*Class I products only*)
- 4 Connect the clip end continuity lead to the ground pin of the DUT. (*Class I products only*)
- 5 Connect the clip end of the high voltage lead to the current carrying conductors of the DUT's circuitry.
- 6 Connect the clip end of ground return lead to the exposed or dead metal chassis of the DUT.

Exposed Metal Chassis Setup (Class I Products)

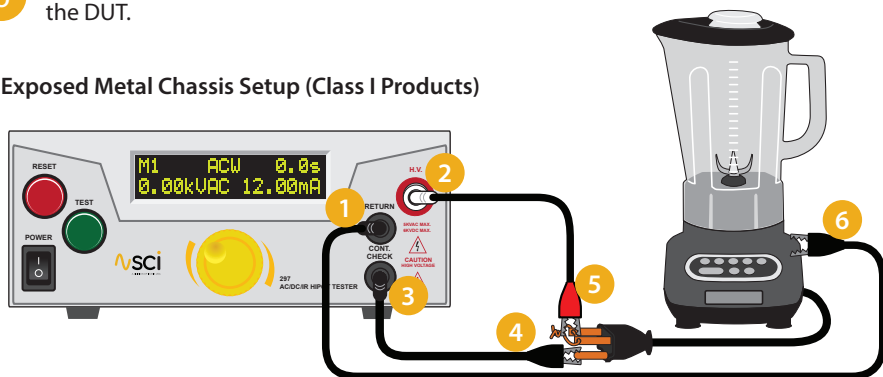

Non-Exposed Metal Chassis Setup (Class II Products)

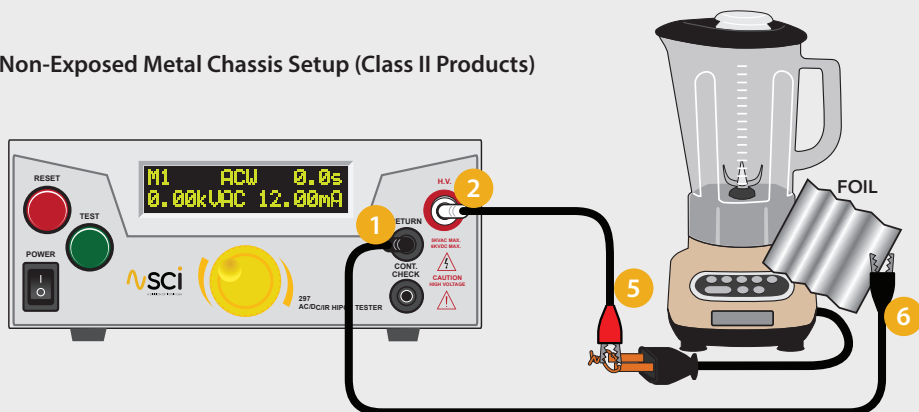

If your chassis does not have any exposed metal, you can wrap the enclosure of the DUT in foil and then connect the return lead to the foil.



WARNING: DO NOT TOUCH THE DEVICE UNDER TEST ONCE YOU START THE TEST.

CONDUCT A TEST

1

Connect the Interlock Disable Key (P/N 9910040-01) to the Signal Input connector on the rear panel of the tester. If you're not utilizing a DUT enclosure (P/N 99-10715-01) or other safety device, **the Interlock Disable Key is required in order to run a test.**



2

With the tester set to the desired test type and your DUT correctly connected to the tester, you are now ready to start testing.

3

If the Continuity function is ON and the resistance of the ground circuit is less than the Max Resistance setting, the green TEST button will illuminate.

4

Push the green TEST button on the front panel. The DUT is tested for a duration equal to the Ramp and Dwell/Delay settings.



TEST RESULTS

PASS: If the DUT passes the test, you will hear a short audible beep and the display will indicate the test results.

FAIL: If a failure occurs, you will hear a long audible alarm and the red flashing indicator will light up. To stop the alarm press the red RESET button.

M1 Hi-Lnt 0.5s
1.24kVA 10mΩ

Pass/Fail Indication Screen

If a failure occurs, a failure code will appear on the screen. Consult your product manual to determine the meaning of your failure code.



See How Simple Using
Your Tester Can Be



Watch the Quick
Start Video



Testers For Electrical Safety Compliance

